

(21)

I 26088

CERTIFICATE

Certified that the specification No. OFPM/R&D/SP/MPV/
STRETCHER (MEDICAL PURPOSE)/015 (Specification of
Stretcher (medical purpose) for MPV) contains 03 pages
and they have been serially numbered from page No: 1 to
page No.: 3.



B.P. BABU
JOINT GENERAL MANAGER
ORDNANCE FACTORY, MEDAK

MASTER COPY

SPECIFICATION NO. : OFPM / R&D / SP / MPV / STRETCHER (MEDICAL PURPOSE) / 015

SPECIFICATION OF STRETCHER (MEDICAL PURPOSE) FOR MPV

(Page No. - 1)

1 SCOPE:

Stretcher (medical purpose) will be fitted in special type automobile vehicle to use carry the injured personnel while any disaster like accident, firing attack, mine attack is occurred.

It should be light in weight, durable, convenient and easy to handle. At the same time it should be strength enough to carry injured persons (approximately 100 kgs.) safely.

It should be preferably foldable type in length wise and widthwise due to space restriction to mount the stretcher in the automotive vehicle.

2 DESCRIPTION OF THE STRETCHER (MEDICAL PURPOSE) ::

a) Maximum sizes of the stretcher : (Length x Width)

2150 ± 50mm X 560 ± 20mm

b) Side Poles :

Length of the side poles : 2150 ± 50mm

Dia / size of the poles : Ø 32 ± 2mm x 2 +1 mm thick

Material of the Poles : Light weight material preferably aluminum

Coating/Painting of the Poles: Any colour preferably olive green/black

Ends of the Poles : PVC cover at the ends of the side poles for proper grip.

c) Stretcher Cloth :

Sizes of the cloth : (Length x Width)


1860mm ± 50mm X 560 ± 20mm

Material of the cloth : Nylon / canvass

Colour of the cloth : Any colour preferably olive green/black

d) Legs : Necessary Legs are to be provided to keep the stretcher about

140mm ± 20mm above the ground lever.


(B.P. BABU)

JT. GENERAL MANAGER

MASTER COPY

(Page No.: 2)


- e) Belts : Proper belts are to be provided to tie up the patient after lay down on the stretcher and to tie up the complete stretcher after folding.
- f) Both the poles are to be properly connected by metal connectors / strips.
- g) Side Poles are to be foldable (at least one fold) in lengthwise.
- h) Stretcher to be foldable (at least one fold) in widthwise also.
- i) Folding mechanism is manufacturers choice subject to end use.
- j) Weight of the component should be about 7 ± 1 kg.

General Notes:

1. Supplier has to submit the broacher for technical and other details regarding his product for consideration while finalizing the case.
2. Supplier has to submit the pilot sample before bulk supply.
3. After Pilot sample acceptance only bulk has to supply.
4. Supplier has to submit the test certificate from the manufacturer.
5. Supplier has to give guarantee for the product for one year from the date of supply.
6. Sketch of the stretcher (page No. 3) is enclosed for reference and guidance for the supplier. However the supplier can quote his own product details.
7. All the items shall be identical and same colour in the supplied lot as per Specification.

INSPECTION:

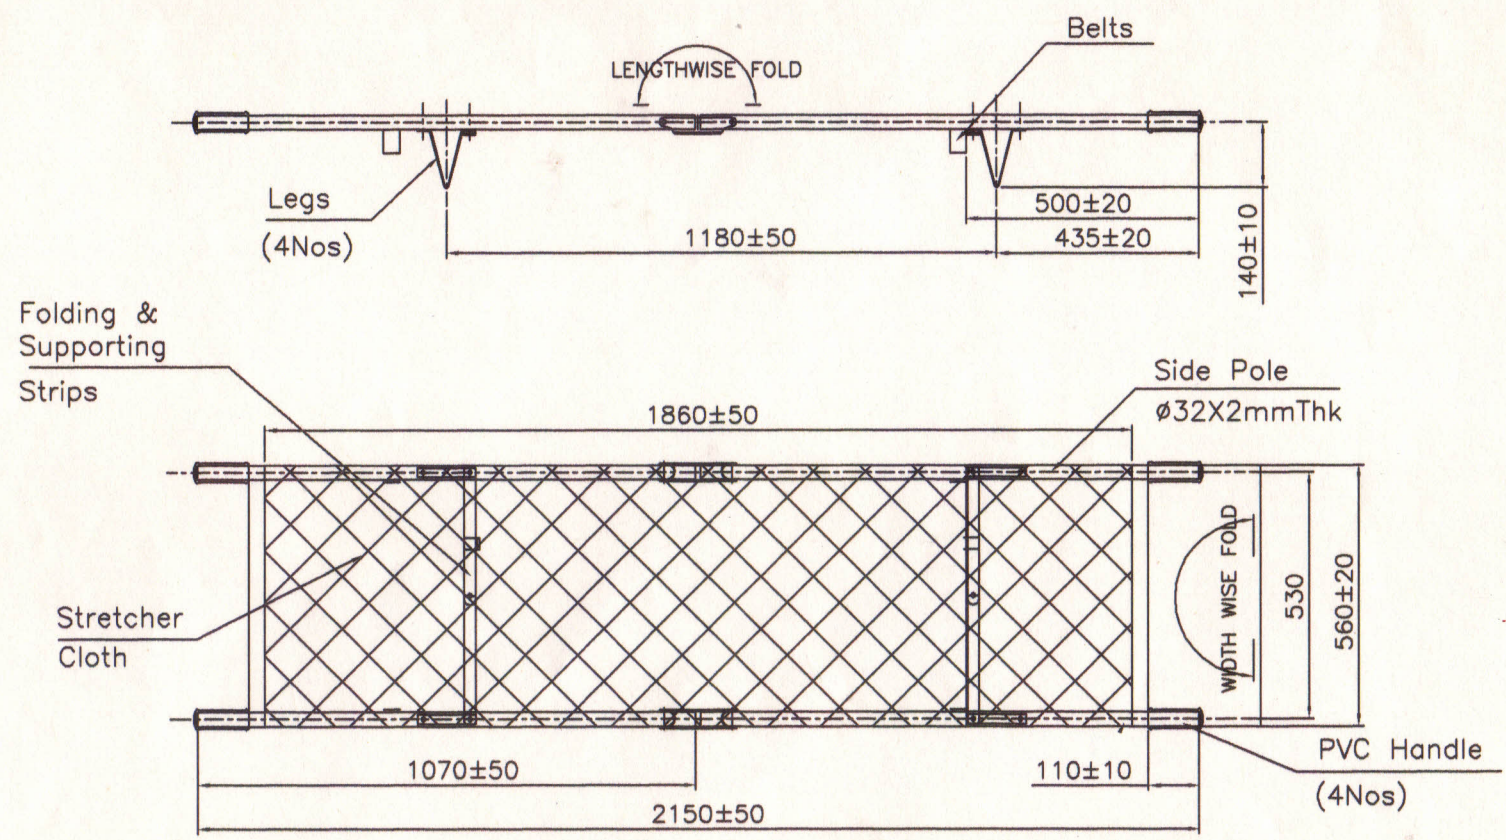
GM / OFPM or his authorized representative at OFMK. The inspector will check all (100%) items.


(B.P. BABU)
JT. GENERAL MANAGER


MASTER COPY

I 26088

SKETCH OF STRETCHER (MEDICAL PURPOSE)



- NOTE:
1. ALL DIMENSIONS ARE IN MM.
 2. DIMENSIONS ARE GIVEN FOR REFERENCE ONLY.


B.P. BABU
JOINT GENERAL MANAGER

MASTER COPY

SHEET NO: 3